




Clearview Hood & Scavenging Circuit Cleaning and Sterilisation Instructions

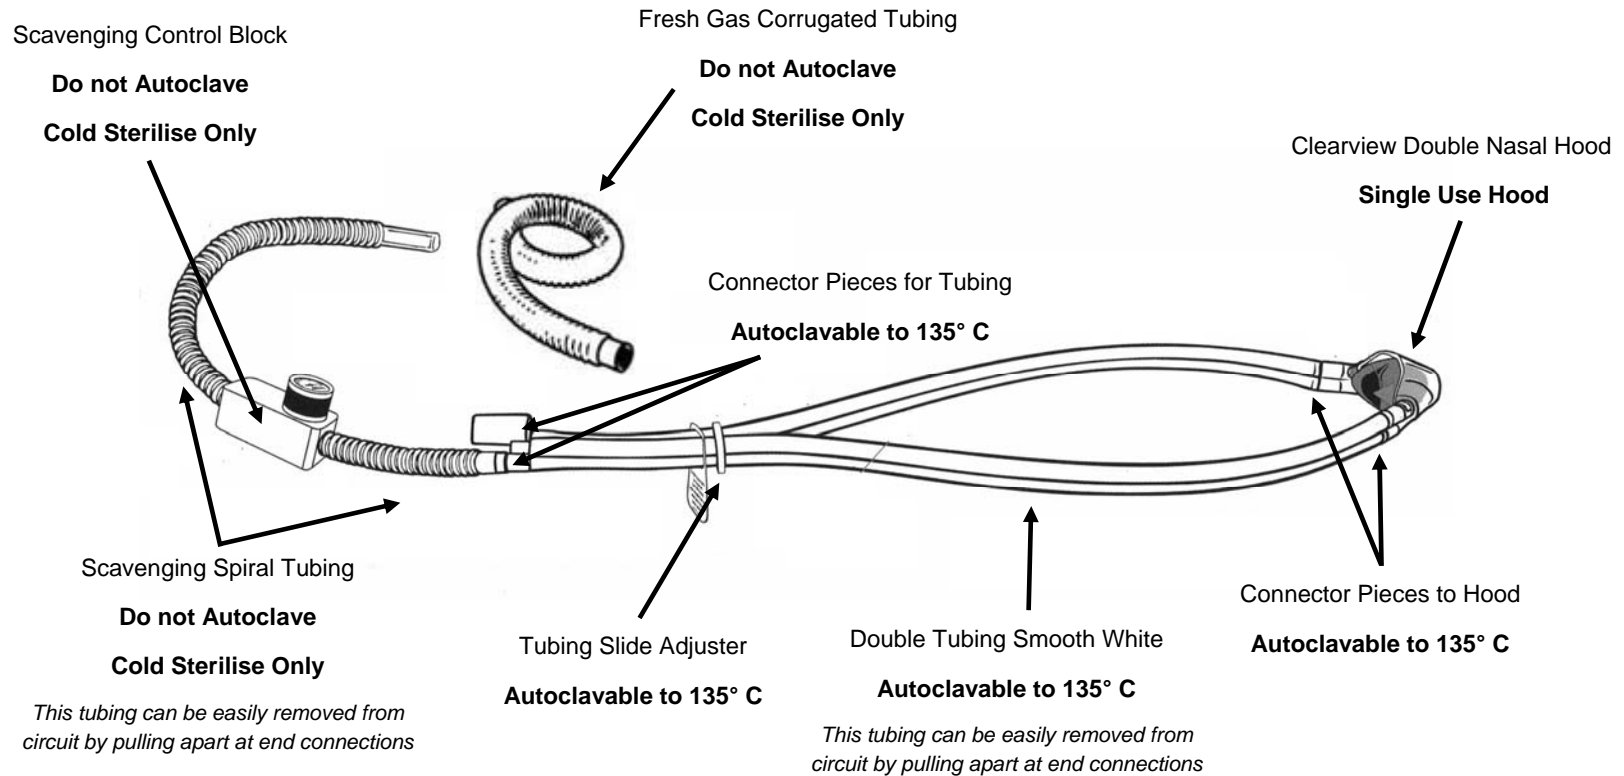


Information_accutronclearviewcircuit_sterilisation0714.pub

Ritter Dental AUSTRALIA | 29/55-59 Norman St Peakhurst NSW 2210 Australia | PO BOX 30, Mortdale NSW 2223

Phone (02) 9153 6700 | Fax (02) 9153 6677 | email: office@ritterdental.com.au | www.ritterdental.com.au



PIP+ Hood & Scavenging Circuit Cleaning and Sterilisation Instructions

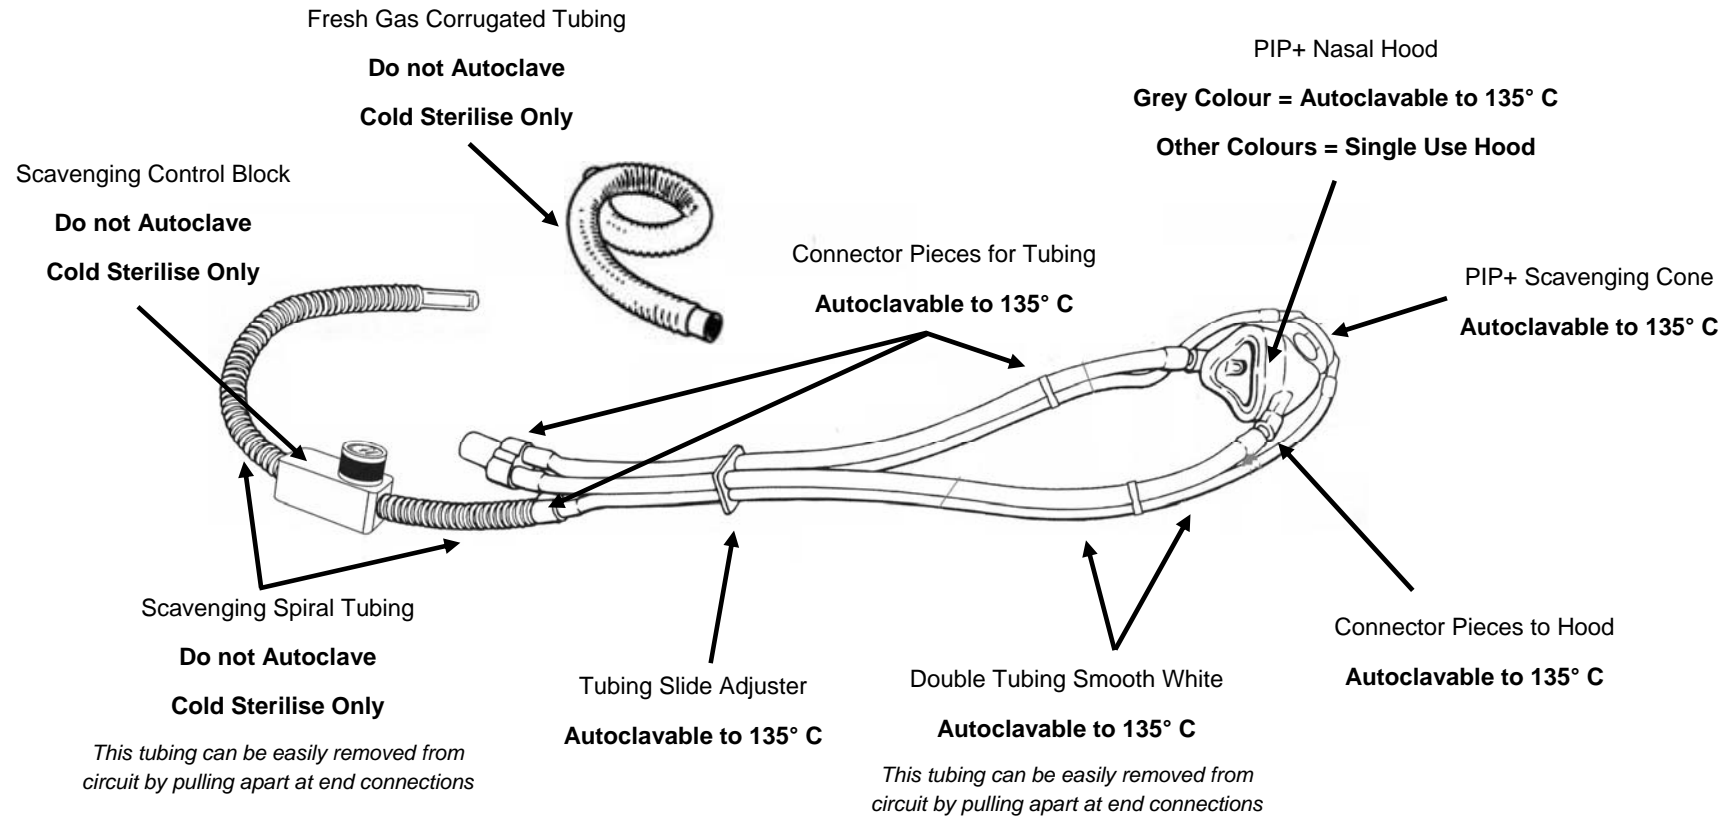

Information_accutronclearviewcircuit_sterilisation0714.pub

Ritter Dental AUSTRALIA | 29/55-59 Norman St Peakhurst NSW 2210 Australia | PO BOX 30, Mortdale NSW 2223

Phone (02) 9153 6700 | Fax (02) 9153 6677 | email: office@ritterdental.com.au | www.ritterdental.com.au